NewTec Scientific

www.newtec.fr

CATHODYNE

Revolution of Optical Cathodoluminescence

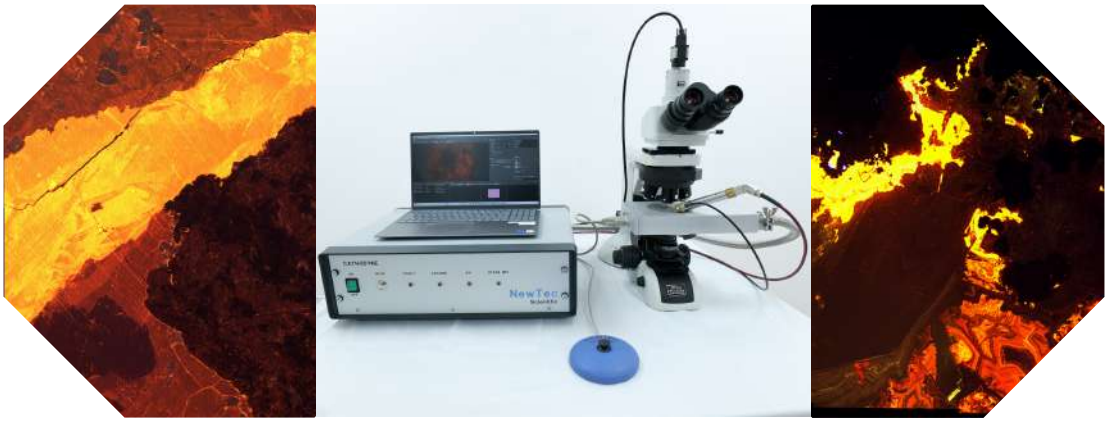

Plasma power controlled & stabilized

Two CL levels:

1.Surfacic

2.Volumic

15 min
To acquire a Thin Section

CL thick samples up to 20mm

Without removing the sample 3 data:

CL / LPA / Spectrometry

Complete thin Section

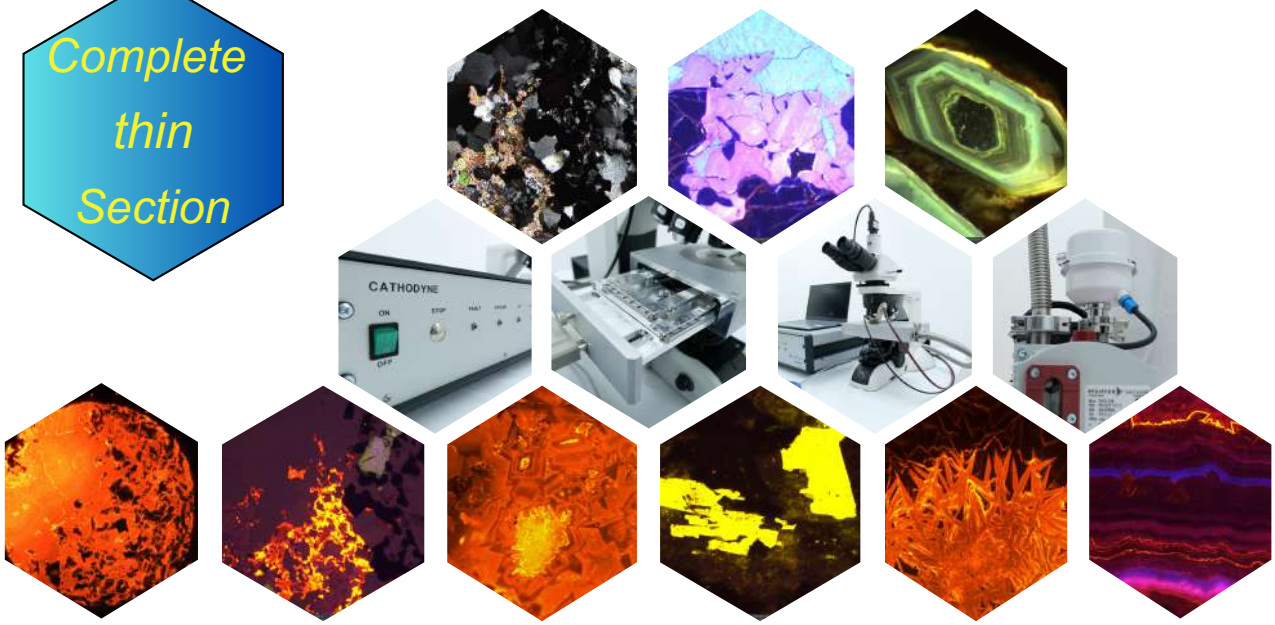

2 route de Sommières – F-30820 CAVEIRAC – Tel: +33 (0)4 66 62 33 04 - contact : ste@newtec.fr